

s032-04 Valida

Data validation

User manual

INDEX

1	INTRODUCTION	2
1.1	DOCUMENT PURPOSE.....	2
1.2	COVERAGE OF THE MANUAL.....	2
1.3	GENERAL OVERVIEW	2
2	ACCESS TO THE DATABASE.....	3
2.1	USER LIMITATIONS	3
3	APPLY THE VALIDATION TO A MEASURE	4
3.1	VALIDATION CRITERIA	5
3.2	BYPASS OF THE VALIDATION	6
4	PROGRAM SET UP	6
5	MEASURES MANAGEMENT	7
5.1	STATION(S) SELECTION	7
5.2	THE CALENDAR	8
5.3	THE TABLE OF THE MEASURES	9
5.4	VALIDATION/UNVALIDATION OF THE DATA	9
5.5	DATA CORRECTION.....	11
5.5.1	<i>Linear interpolation</i>	11
5.6	UNVALIDATE THE DATA	11

1 Introduction

1.1 Document purpose

This document is the user manual for the software module MeteoGIS, which can be used for the presentation of the meteorological data in a geographic coordinate system.

1.2 Coverage of the manual

Valida is a project that grew up during the time, with always new features developed for the needs of the different plants. This means that some function of the software may not be used in your project. In particular, all the features useful to the current plant are explained in this manual. All other features of the software are reserved for different type of installations and, so, may do not be available.

1.3 General overview


The software module Valida use the Meteonet LT package database:

- Configuration database
- Data database

It access the databases using the Microsoft Data Access Components, distributed with the Meteonet LT package. The configuration database contains all the information about the stations, the measures, the scheduled activities, the user and their alarms notification method, while the data database contains all the measures acquired by the data loggers.

Using the data access components brings two important features:


- ✓ Valida is independent from the type of database used
- ✓ Better performance in network applications

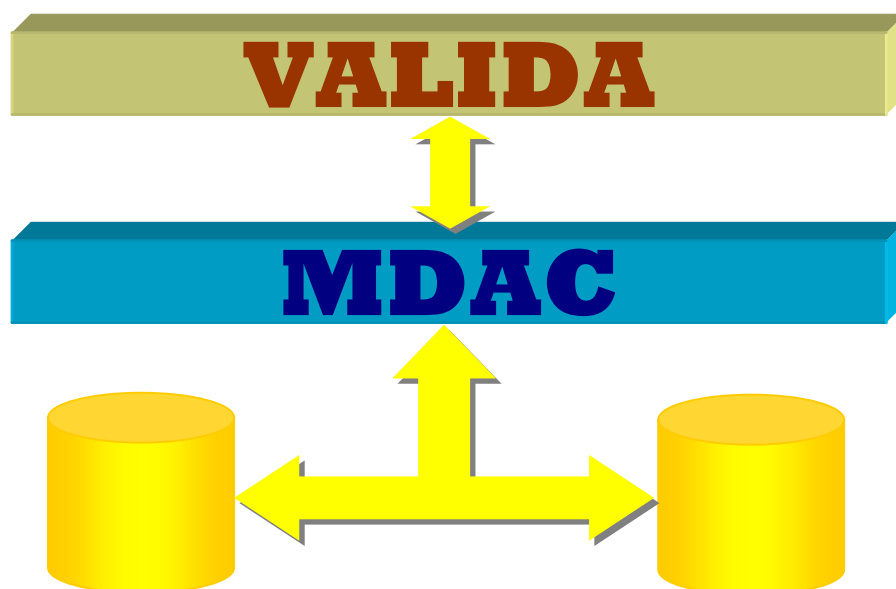


Picture 1

2 Access to the database

On the start up of Valida, the user is prompted to select the database on which he want to operate (Picture 1). Usually this is the data database of Meteonet LT package. To access this database, the user must insert a valid username and password (Picture 2). The accounts are stored in the configuration database of Meteonet LT and can be configured with the software module GestConf (see the GestConf manual).

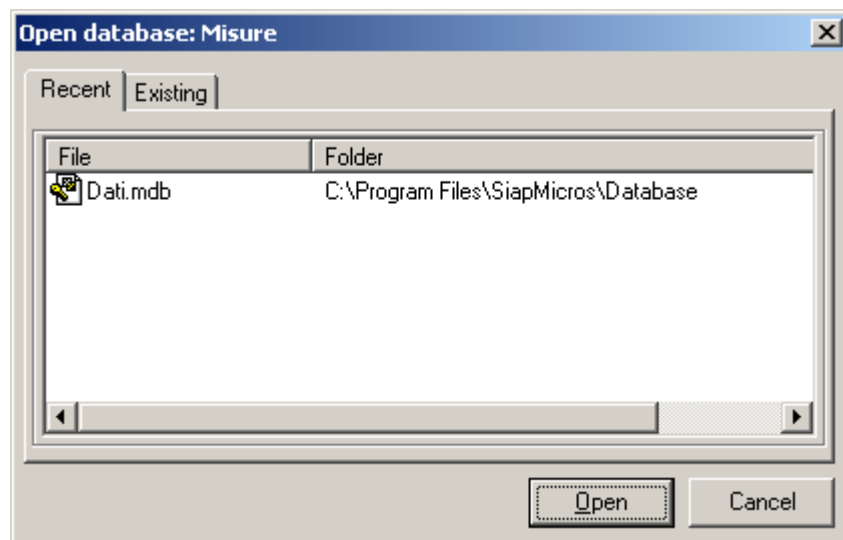

Picture 2

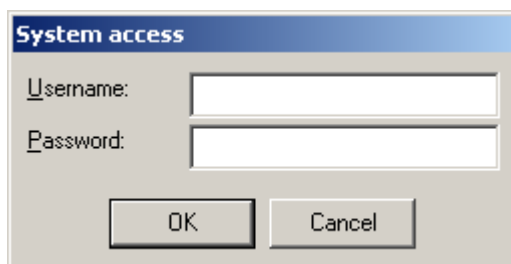

Picture 3

2.1 User limitations

Only user with administrative privilege will be allowed to modify the data with the software Valida.


3 Apply the validation to a measure

The validation can be applied to the measure using the software GestConf for the configuration of the network. In particular the procedure steps are:

- ✓ Start GestConf and access the database (with the same procedure seen in before)
- ✓ Select the button **Anl measure** from the toolbar



- ✓ From the next window, select the desired measure, mark the check box **Apply validation filter** (Picture 4) and click the button **Save**

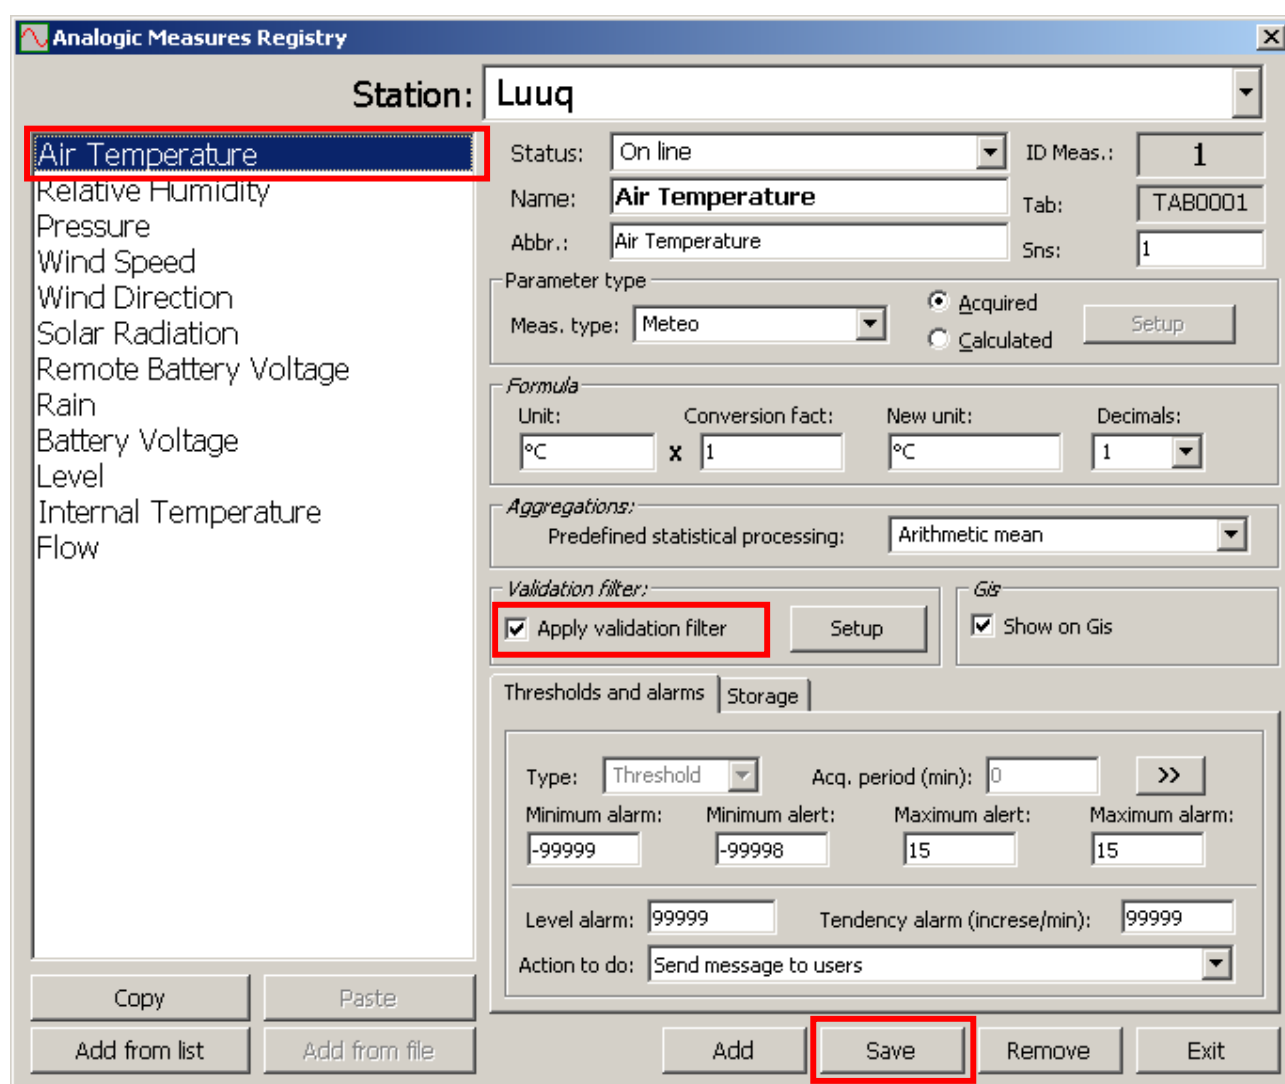

Analogic Measures Registry

Station: **Luuq**

Air Temperature (selected)

Relative Humidity
Pressure
Wind Speed
Wind Direction
Solar Radiation
Remote Battery Voltage
Rain
Battery Voltage
Level
Internal Temperature
Flow

Status: **On line** ID Meas.: **1**

Name: **Air Temperature** Tab: **TAB0001**

Abbr.: **Air Temperature** Sns: **1**

Parameter type: **Acquired**

Meas. type: **Meteo**

Formula:

Unit: **°C** Conversion fact: **1** New unit: **°C** Decimals: **1**

Aggregations:

Predefined statistical processing: **Arithmetic mean**

Validation filter:

☒ **Apply validation filter**

GIS:

☒ **Show on Gis**

Thresholds and alarms

Type: **Threshold** Acq. period (min): **0**

Minimum alarm: **-99999** Minimum alert: **-99998** Maximum alert: **15** Maximum alarm: **15**

Level alarm: **99999** Tendency alarm (increase/min): **99999**


Action to do: **Send message to users**

Buttons: Copy, Paste, Add from list, Add from file, Add, **Save**, Remove, Exit

Picture 4

3.1 Validation criteria

The measures are validated against different criteria, that can be configured clicking on the button **Setup** of the window shown in Picture 4.

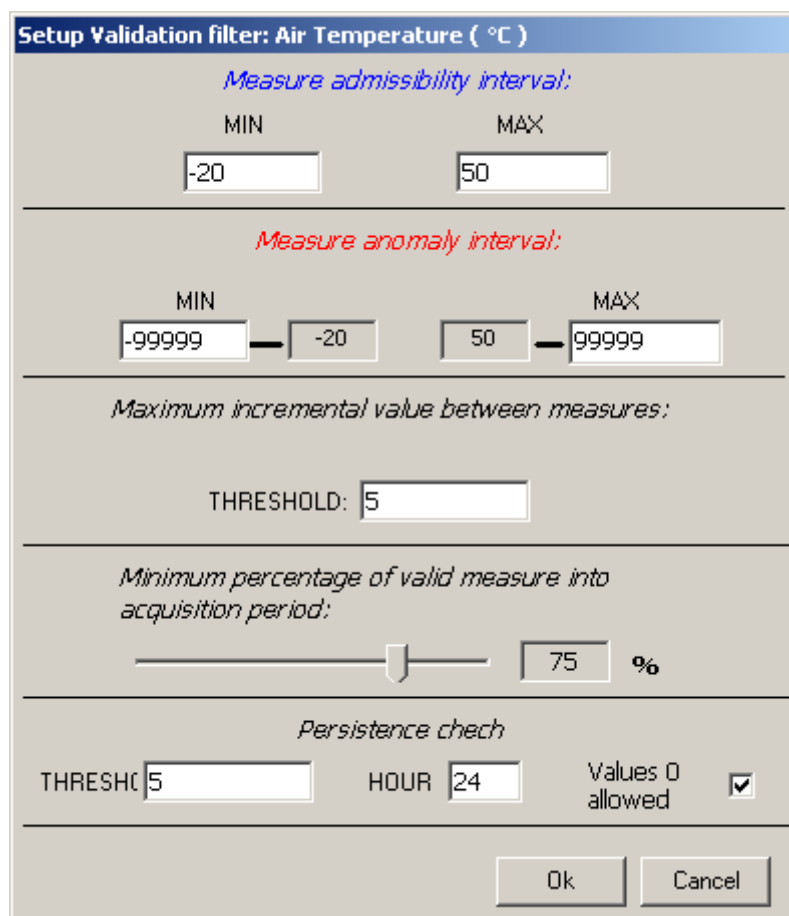

Setup Validation filter: Air Temperature (°C)

Measure admissibility interval:

MIN: -20 MAX: 50

Measure anomaly interval:

MIN: -99999 MAX: 99999

Intermediate values: -20, 50

Maximum incremental value between measures:

THRESHOLD: 5

Minimum percentage of valid measure into acquisition period:

Slider: 75 %

Persistence check

THRESHOLD: 5 HOUR: 24 Values 0 allowed: ☒

Ok Cancel

Picture 5

- ✓ **Measure admissibility interval:** specifies the minimum and maximum values allowed for the measure
- ✓ **Measure anomaly interval:** used for water chemical parameters
- ✓ **Maximum incremental value between measures:** specifies the maximum difference allowed between two consecutive values
- ✓ **Minimum percentage of valid measure into acquisition period:** each measure stored by the data logger is the result of the average of more values. This parameters specifies the minimum percentage of valid measures (according to the validation thresholds in the data logger) the data logger must have when evaluate the average.
- ✓ **Persistence check:** this parameter specifies that in the interval of n HOURS, the difference between minimum and maximum values of the measure must be at least THRESHOLD. In the example of Picture 5, the measure is valid if in 24 hours the difference between the minimum and maximum air temperature is at least 5 Celsius degrees. The control is bypassed if the measure is always zero and the checkbox **Value 0 allowed** is marked.


3.2 Bypass of the validation

When the validation is applied to a measure, the software Importa, which import the data downloaded from the stations into the data database, will store the data only in the raw field of the database and not in the validated field. Since the data visualization programs DataView and WebView, works with validated data, this means that the new values of the measure will not appear, until an administrator user will validate them following the procedure explained in point 5.5.

If the validation is not applied, the raw values will be automatically stored also in the validated field, and, so, they will be visible in the client programs. In any case the user can operate again on the data with the software Valida, to verify or change them later, without stop the visualization. **This is the suggested solution.**

4 Program set up

To enter the program option, select the main menu command Setup ► Customize. This section allows to customize some parts of the interface. An important parameter is located in the measures tab:

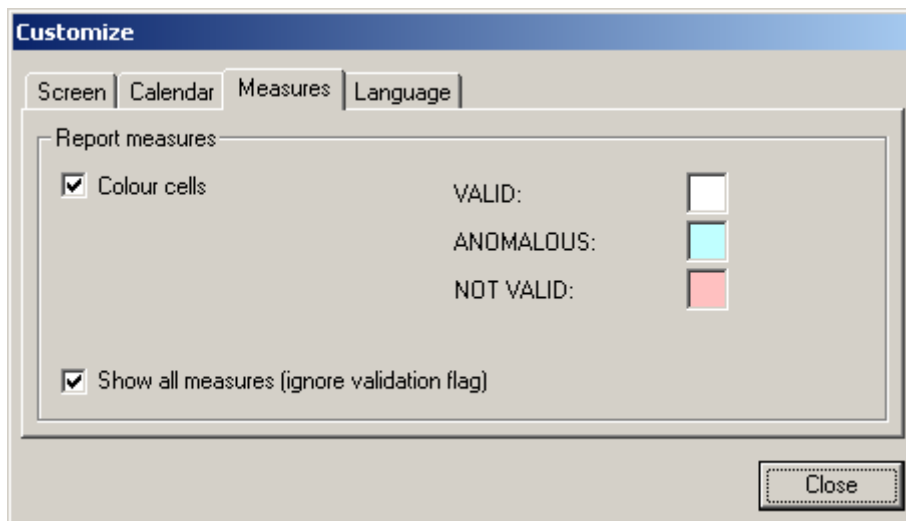

Picture 6

Show all measures (ignore validation flag): if this check box is marked, the user can operate on all the measures, even if they do not have the validation. So this check box should be marked in case of validation bypass. Otherwise the user will be able to operate only with the measures to which the validation has been applied.

5 Measures management

This section describes the detailed sequence for the validation of the data.


5.1 Station(s) selection

To operate on the data, the first step to do is select the stations to manage. The software Valida works basically with two type of windows: the calendar (see point 5.2) and the measures table (see point 5.3). The user will operate on copies of this windows, one for each station selected. For this reason, from this point on the manual will consider the operations done on only one station.

Click on the button **Stations** (Show ► Stations List...):



and in the following window select the stations to manage:

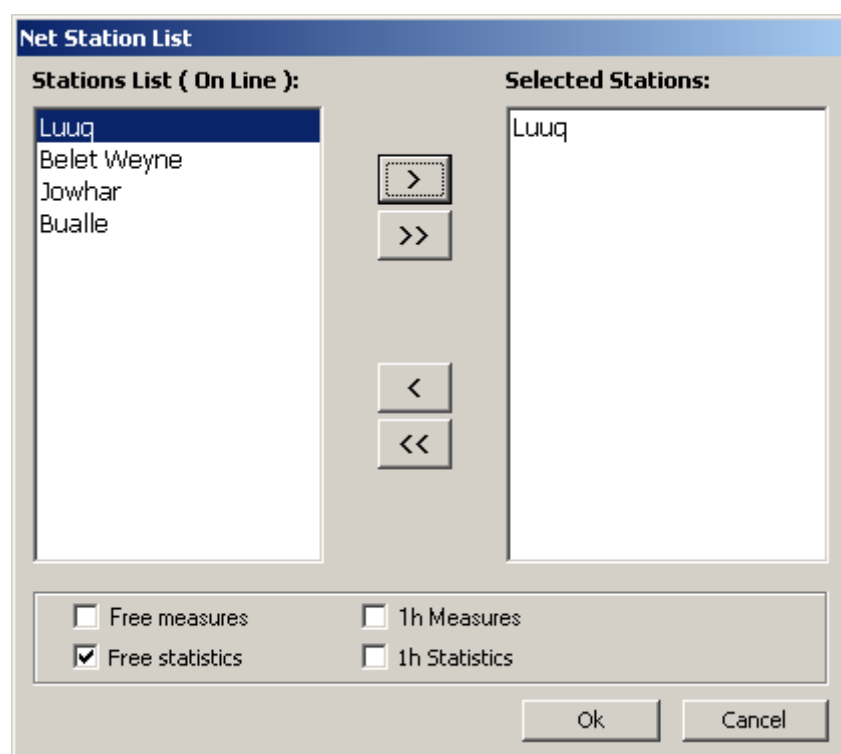

Picture 7



Add the selected station



Add all stations



Remove the selected station



Remove all stations

To manage the data of a day, double click on the day to open the next window which contains the table of the measures.

5.3 The table of the measures

The table of measure shows two columns for each parameter:

- ✓ The raw value: is the original value, as it come from the data logger. It is displayed in bold type font, to indicate that this value cannot be changed
- ✓ The validated value: is the value processed by the user validation and used by the visualization programs. There are two cases:
 - The validation is bypassed (see point 3.2): if the program setup allows to display all the measures, this column will be filled with the raw value
 - The measures must be validated: if the values match the validation criteria, the software will propose the raw value, otherwise this column will be empty. In any case the measure must be manually validated to be shown in the visualization programs.

An additional column is present, with the following meaning:

- N** value not present. The user did not validate the data
- N** value not present. The user already validated the data
- Y** value present. The user did not validate the data
- Y** value present. The user already validated the data

The raw values are displayed in bold type font, to indicate that they cannot be changed. If the value match all the validation criteria specified in the configuration (see point 3.1), the software Valida suggest the same value in the validated data column, otherwise this column will be empty (Picture 10).

In the measures window all operations are done in the temporary memory of the server. To make the changes in the physical database it is necessary to confirm with the button **Confirm Validation !!**.

5.4 Validation/Unvalidation of the data

The procedure for data validation consists in the following steps:

- ✓ Select the values to validate: it is possible to select a single value, clicking on it, or a set of values, clicking on the first and dragging the mouse to the last (keeping the button clicked), but always in the same column.
- ✓ Right click on the selected data and give the command **Set up Validate**
- ✓ In the window of Picture 9 select the option VALID to validate, NOT VALID to invalidate the measure
- ✓ Click the **Apply** button
- ✓ If the NOT VALID option was selected, the value in the validated data column will be deleted

The procedure must be repeated for all the data. When done, confirm with the button **Confirm Validation !!**. Now, clicking on the **Refresh** button in the calendar window, the processed day will appear in green color.

Setup...

Measure: Air Temperature(°C) (RAW)

Day: 25-Jul-2008

From: 08.00 To: 08.00

Setup as: ☒ VALID ☐ NOT VALID

Add/Subtract :

Multiply:

Cancel Apply

Picture 9

Measures Libre : Luuq

Air Temperature(°C) (RAW)

01:00

Records: 96

			Air Temperature (RAW)	Air Temperature (V.D.)	Air Temperature (RAW)	Relative Humidity (RAW)	Relative Humidity (V.D.)	Relative Humidity (RAW)	Pressure (RAW)	Pressure (V.D.)	Pressure (RAW)	Wind Speed (RAW)	Wind Speed (V.D.)	Wind Speed (RAW)	Wind Direction (RAW)	Wind Direction (V.D.)	Wind Direction (RAW)	Solar Radiation (RAW)	Solar Radiation (V.D.)	Solar Radiation (RAW)	Remote Battery Voltage (RAW)
21-May-2008	09.30	10.00			N			N			N			N			N			N	
21-May-2008	09.45	10.00			N			N			N			N			N			N	
21-May-2008	10.00	10.00	18.7	18.7	Y			N	824.	Y	1.7	1.7	Y	16.	16.	Y	531.	531.	Y		
21-May-2008	10.15	11.00			N			N			N			N			N			N	
21-May-2008	10.30	11.00			N			N			N			N			N			N	
21-May-2008	10.45	11.00			N			N			N			N			N			N	
21-May-2008	11.00	11.00	19.3	19.3	Y	67.6	67.6	Y	824.	Y	1.	1.	Y	62.	62.	Y	472.	472.	Y		
21-May-2008	11.15	12.00			N			N			N			N			N			N	
21-May-2008	11.30	12.00			N			N			N			N			N			N	
21-May-2008	11.45	12.00			N			N			N			N			N			N	
21-May-2008	12.00	12.00	20.4		N	63.5	63.5	Y	823.	Y	1.6	1.6	Y	62.	62.	Y	523.	523.	Y	13.	
21-May-2008		13.00			N			N			N			N			N			N	
21-May-2008		13.00			N			N			N			N			N			N	
21-May-2008		13.00			N			N			N			N			N			N	
21-May-2008	13.15	14.00			N			N			N			N			N			N	
21-May-2008	13.30	14.00			N			N			N			N			N			N	
21-May-2008	13.45	14.00			N			N			N			N			N			N	
21-May-2008	14.00	14.00	23.		N	50.8	50.8	Y	822.	Y	2.5	2.5	Y	51.	51.	Y	841.	841.	Y	13.	
21-May-2008	14.15	15.00			N			N			N			N			N			N	
21-May-2008	14.30	15.00			N			N			N			N			N			N	
21-May-2008	14.45	15.00			N			N			N			N			N			N	
21-May-2008	15.00	15.00	23.4		N	49.	49.	Y	821.	Y	2.9	2.9	Y	50.	50.	Y	766.	766.	Y	13.	
21-May-2008	15.15	16.00			N			N			N			N			N			N	
21-May-2008	15.30	16.00			N			N			N			N			N			N	
21-May-2008	15.45	16.00			N			N			N			N			N			N	
21-May-2008	16.00	16.00	23.6		N	48.	48.	Y	821.	Y	2.3	2.3	Y	63.	63.	Y	564.	564.	Y	13.	
21-May-2008	16.15	17.00			N			N			N			N			N			N	
21-May-2008	16.30	17.00			N			N			N			N			N			N	
21-May-2008	16.45	17.00			N			N			N			N			N			N	
21-May-2008	17.00	17.00	23.1		N	48.5	48.5	Y	821.	Y	2.2	2.2	Y	57.	57.	Y	336.	336.	Y	13.	
21-May-2008	17.15	18.00			N			N			N			N			N			N	
21-May-2008	17.30	18.00			N			N			N			N			N			N	
21-May-2008	17.45	18.00			N			N			N			N			N			N	
21-May-2008	18.00	18.00	22.1		N	51.5	51.5	Y	821.	Y	2.1	2.1	Y	57.	57.	Y	72.	72.	Y	12.	
21-May-2008	18.15	19.00			N			N			N			N			N			N	
21-May-2008	18.30	19.00			N			N			N			N			N			N	
21-May-2008	18.45	19.00			N			N			N			N			N			N	

Measures out of validation criteria

Load measure ...

Previous

Next

1 / 1

ReOpen

Confirm Validation !!

Cancel

Picture 10

5.5 Data correction

Data correction allows to input manually values for the parameters. It can be done in two different ways, even after the validation.

- ✓ Manual input: it can be done only on a single value. Select it in the validated data column and enter the correct value. Confirm it with Return key
- ✓ Span/offset correction: it can be done on a single value or on a set of values. Select the values to correct, right click on them and select the command Set up Validate. In the window shown in Picture 9 enter a value in one of the fields **Add/Subtract** or **Multiply**. The software will update automatically all the selected values applying the formula. The multiply field has higher priority on the offset: if the user enter both the field, only the multiply will be applied.

5.5.1 Linear interpolation


Linear interpolation is a particular way of automatic correction. It works on a set of value and allows to calculate new values in the interval that stay on a straight line. See the example table below:

2.5		2.5
<not present>		7.0
<not present>		11.4
<not present>		15.9
20.4		20.4

5.6 Unvalidate the data

It is possible to remove the validation for all the data of one or more stations in a specified period. With this operation the user can declare that the data in the selected period, for the selected stations are not valid and, so, they will not be visible anymore in the visualization programs, until the user will confirm the validation again. For this reason, it is considered a critical operation.

To invalidate the data, select the command from main menu Tools ► Remove validation flags. In the window of Picture 11 select the period, which can be a single day or an interval of more days, and the stations whose data will be invalidated. Then click on the button **Apply** to invalidate the data. The button **Cancel** will close the window.

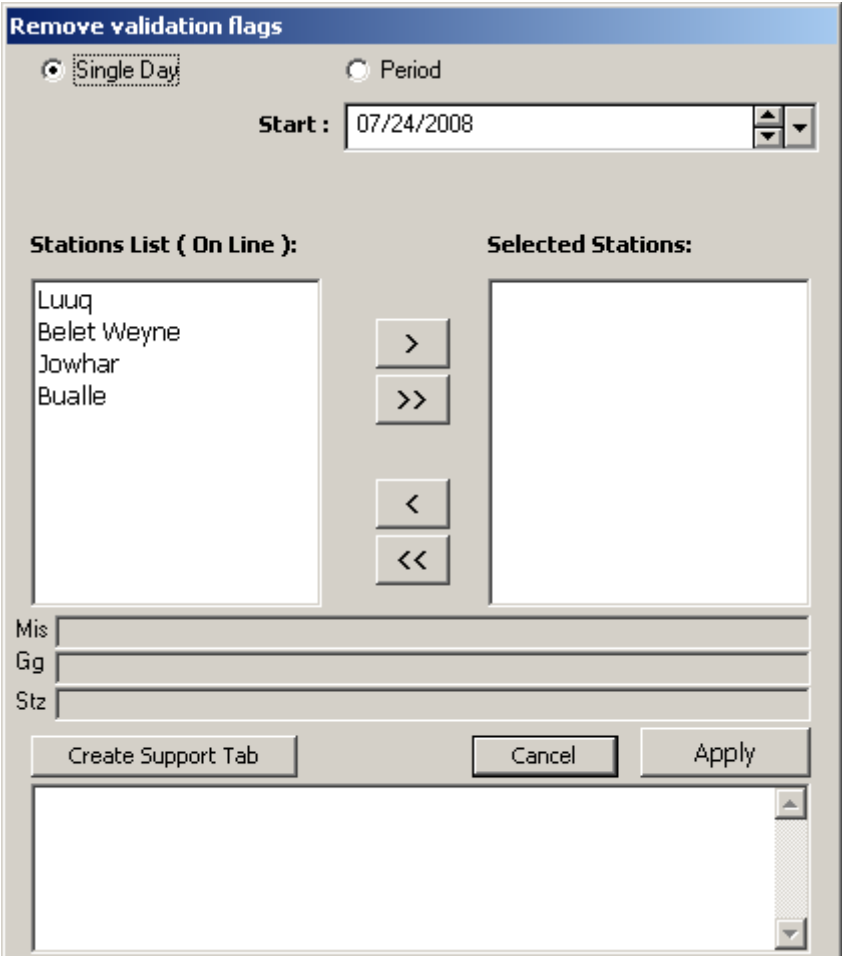

Remove validation flags

☒ Single Day ☐ Period

Start : 07/24/2008

Stations List (On Line):

- Luuq
- Belet Weyne
- Jowhar
- Bualle

Selected Stations:

Mis

Gg

Stz

Create Support Tab Cancel Apply

Picture 11